



# Nature Line CT Phantom – Extremity



*Experts in medical education  
since 1950*



**ERLER ZIMMER**

## Extremity Phantom



Size	Approx. 6 x 11 x 20 cm
Weight	Approx. 0.5 kg

Hand phantom with two metacarpal fractures. Attenuation values are calibrated to be equivalent to human tissue at 120 kVp CT imaging. Calibration to other spectrum energies (e.g., 100 kVp CT imaging) is possible upon request.

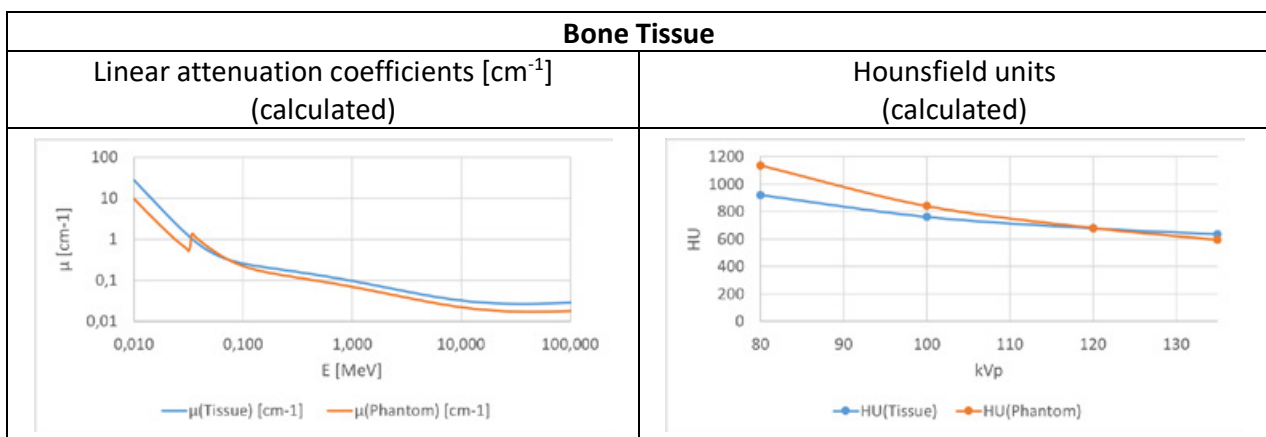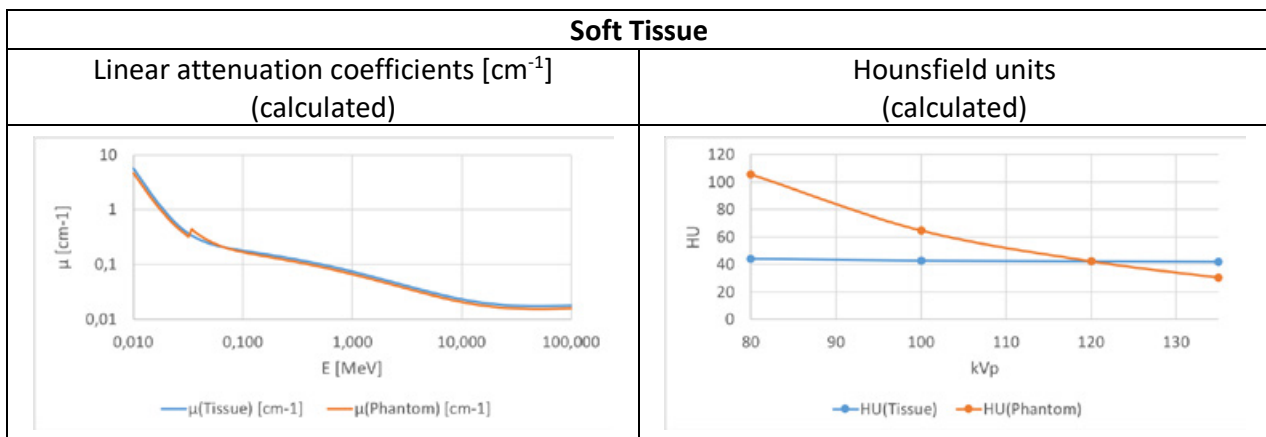

*Tissue Reference:* Woodard HQ, White DR. The composition of body tissues. Br J Radiol. 1986;59(708):1209-18.

### General indications

- Phantoms are manufactured of a cellulose-polymer composite material with similar properties to hardwood. If treated carefully, they will last for a long period.
- The phantoms are coated with a protective layer. If the protective layer is unharmed, the phantoms can be cleaned using a damp cloth (water or mild detergent).
- Protect from direct sunlight.
- Maintain a storage temperature of 10 °C to 30 °C.
- If the phantom is exposed to temperatures below -10 °C or above 45 °C, it can be seriously damaged.
- The phantom is not equipped for dose measurements with dosimeters and it is not suited for material characterization with dual energy CT.
- Air voids are filled with cellulose-polymer composite of approx. -80 HU.