

# Sterile CT Scanner Drape

Surgical and non-surgical related infections can affect a patient's quality of life and create stress for patients and their families. And they place a huge operational and financial burden on health care systems and providers. Using evidence-based practices to reduce skin microbes – before and during interventional radiology and routine CT imaging – and creating a barrier to microbial migration can help reduce the risk of an infection and increase workflow.

## Easy to Use

- 5 step fold system to maintain sterility
- Intuitive and easy to install

## Safe for Patients and Operators

- Reduces the cross-contamination between patient and procedure
- Absorbent drape which prevents spillage

## Seamless and Reliable Performance


- Can be used on any scanner manufacture
- Collecting bag for excessive fluid spills

## Economical

- Side pockets to increase procedure workflow
- Increases patient through put by reduced cleaning times

TMH will reserve the right on product improvement and product design modification, without previous notification

<b>Drape Dimension</b>	<ul style="list-style-type: none"> <li>• Front Piece 135 x 160 cm</li> <li>• Connected back piece 42 x 45 cm</li> </ul>
<b>Drape</b>	<ul style="list-style-type: none"> <li>• Drape bag size: 31 x 45 cm</li> <li>• 50 drapes per box: 5ply carton</li> <li>• Box dimension: 60 x 48 x 32 cm</li> <li>• Box Weight: 17kg/carton (Net Weight 15kg/carton)</li> </ul>
<b>Material</b>	<ul style="list-style-type: none"> <li>• Fabric: SSPE 90g dark blue hydrophilic PP coated with blue cast film, square dot pattern</li> <li>• Adhesive strips: 2cm blue waterproof adhesive strips</li> <li>• PE films: 0.08mm thickness transparent PE film</li> <li>• Double-sided tape width: 2cm</li> </ul>
<b>Connection</b>	<ul style="list-style-type: none"> <li>• The fabric side is the front side which is ultrasonic heat-sealed with cutter wheel</li> <li>• The film side of the heat-sealed part is pasted with strips</li> <li>• The fabric side of the triangular piece + film side heat-sealing</li> </ul>
<b>Absorption Volume and Saturation</b>	<ul style="list-style-type: none"> <li>• 2 liters on the surface without leakage at maximum saturation for 12 hours</li> <li>• 1 liter in the collection bag without leakage at maximum saturation for 12 hours</li> </ul>

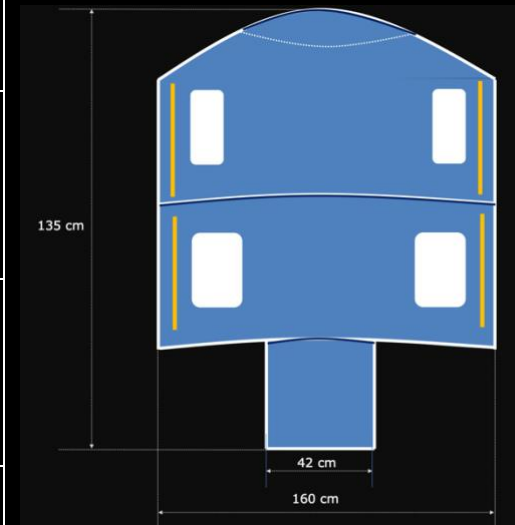

[www.techmed-health.com/drape/](http://www.techmed-health.com/drape/)

**KEY**



Absorbent sterile surface



Clear aperture for laser lights



Adhesive Strips



Ultrasonic heat sealed connections